

## PRODUCT INFORMATION SHEET

### Monoclonal antibodies detecting human antigens

### CD41

FITC RUO REF IQP-551F ▽ 100 tests

RUO **For Research Use Only**

#### Description

**Clone** MEM-06

**Isotype** IgG1

**Specificity** The immunogen used were leukocytes of patient suffering from LGL-type leukaemia. The antibody MEM-06 reacts with CD41 (GPIIb), a transmembrane glycoprotein (integrin family) composed of two chains GPIIba (heavy chain; 120 kDa) and GPIIbb (light chain; 23 kDa).

**Antigen distribution** CD41 is expressed on platelets and megakaryocytes.


**Summary** CD41 antibodies are used for the identification of platelets and the diagnosis of Glanzmann thrombasthenia and leukemia. CD41/CD61 is the major integrin on platelets and is important for platelet adhesion and aggregation. The ligands for CD41/CD61 include fibrinogen, Von Willebrand factor, fibronectin, vitronectin, and thrombospondin [3]. Binding to these ligands depends on the activation state of the platelets [1].

**Applications** Monoclonal antibody CD41, clone MEM-06, can be applied in flow cytometry for analysis of blood or bone marrow samples.

**Usage** All these reagents are effectively formulated for direct immunofluorescent staining of human tissue for flow cytometric analysis using 10  $\mu\text{l}/10^6$  leukocytes for singles and 20  $\mu\text{l}/10^6$  leukocytes in case of dual and triple combinations. Since applications vary, each investigator should titrate the reagent to obtain optimal results.

**HLDA Workshop** Leukocyte Typing Workshop VI, Kobe

**Representative Data** Staining with clone MEM-06 monoclonal antibodies is illustrated by flow cytometry analysis of platelets. Direct staining was performed using 10  $\mu\text{l}$  of FITC-conjugated antibody with 100  $\mu\text{l}$  platelets.

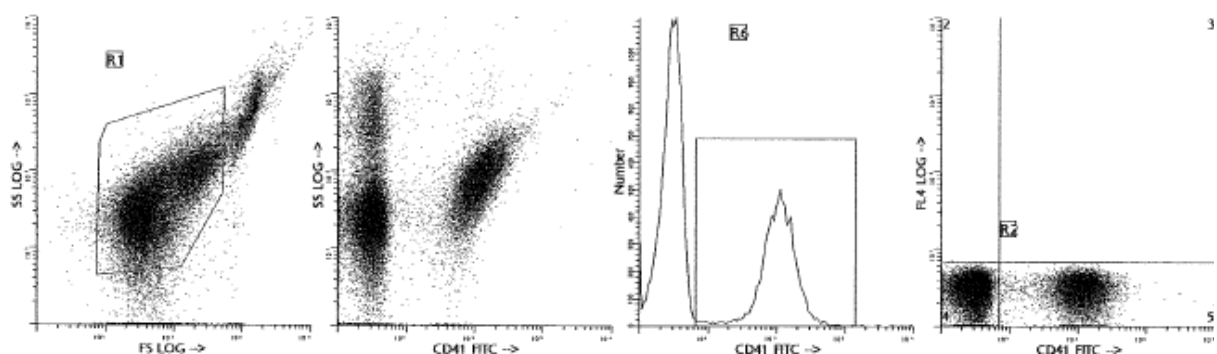

## Limitations

1. Conjugates with brighter fluorochromes, like PE and APC, will have a greater separation than those with dyes like FITC and CyQ. When populations overlap, the percentage of positive cells using a selected marker can be affected by the choice of fluorescent label.
2. Use of monoclonal antibodies in patient treatment can interfere with antigen target recognition by this reagent. This should be taken into account when samples are analyzed from patients treated in this fashion. IQ Products has not characterized the effect of the presence of therapeutic antibodies on the performance of this reagent.
3. Reagents can be used in different combinations, therefore laboratories need to become familiar performance characteristics of each antibody in relation with the combined markers in normal and abnormal samples.
4. Reagent data performance is based on EDTA-treated blood. Reagent performance can be affected by the use of other anticoagulants.

## Reagents and materials required but not supplied

1. Flow cytometer
2. Flow cytometry disposable 12 x 75-mm capped polystyrene test tubes
3. Micropipette with disposable tips
4. Vortex mixer
5. Centrifuge
6. IQ Lyse - erythrocyte lysing solution (IQP-199)
7. IQ Starfiqs - fixation and permeabilization solution (IQP-200)
8. PBS (phosphate-buffered saline)
9. 1% paraformaldehyde solution in PBS (store at 2-8 °C in amber glass for up to 1 week)

## Immunofluorescence staining and lysing protocol

1. Use EDTA blood.
2. Centrifuge the tube 10 minutes (600g). If possible soft start/soft stop procedure.
3. Collect plasma and dilute in PBS (+5 mM EDTA). Total volume is 10 ml.
4. Centrifuge the tube 10 minutes (2000g). If possible soft start/soft stop procedure.
5. Count the cell population on a counter.
6. Dilute to  $1 \times 10^9$  cells/ml in PBS (+5 mM EDTA).
7. Add to 10  $\mu$ l of cell suspension 5  $\mu$ l of human serum (pooled).
8. Add 10  $\mu$ l of the labelled antibody.
9. Incubate for 30 minutes at room temperature.
10. Add 2 ml of PBS (+5 mM EDTA).
11. Centrifuge the tube 5 minutes (2000g). If possible soft start/soft stop procedure.
12. Discard supernatant.
13. Resuspend the pellet in 300  $\mu$ l PBS (+5 mM EDTA).
14. Choose log amplification for morphological parameters FSC/SSC.



## Handling and Storage

Antibodies are supplied either as 100 tests per vial (1 ml) for singles or 50 tests per vial (1 ml) for dual and triple combinations. They are supplied in 0.01 M sodium phosphate, 0.15 M NaCl; pH 7.3, 0.2% BSA, 0.09% sodiumazide ( $\text{NaN}_3$ ). Store the vials at 2-8 °C. Monoclonal antibodies should be protected from prolonged exposure to light. Reagents are stable for the period shown on the vial label when stored properly.

**Warranty** Products sold hereunder are warranted only to conform to the quantity and contents stated on the label at the time of delivery to the customer. There are no warranties, expressed or implied, which extend beyond the description on the label of the product. IQ Products is not liable for property damage, personal injury, or economic loss caused by the product.

## Characterization

To ensure consistently high-quality reagents, each batch of monoclonal antibody is tested for conformance with characteristics of a standard reagent. Representative flow cytometric data is included in this data sheet.















**Warning** All products contain sodiumazide. This chemical is poisonous and hazardous. Handling should be done by trained staff only.

---

## References

1. Barclay, A.N., et al., 1997, The Leucocyte Antigen Factsbook. Academic Press. London
  2. Kishimoto, et al., eds. 1998, Leucocyte Typing VI. Kobe, Garland Pub. Inc.
  3. Phillips, D.R., et al., 1991, Cell 65, 359-362
- 

## Explanation of used symbols

	Consult instructions for use
	Catalogue number
	Sufficient for
	In Vitro Diagnostic medical device
	Caution, consult accompanying document
	Keep away from (sun)light
	Biological risks
	Temperature limitation (°C)
	For Research Use Only
	Batch code
	Use by yyyy-mm-dd
	Manufacturer
	Authorized Representative in the European Community
	Conformité Européenne (European Conformity)

		<b>Label - tandem</b>	<b>Ex -max (nm)</b>	<b>Em -max (nm)</b>
P	PURE	purified material	-	-
F	FITC	FITC	488	519
R	R-PE	PE	488, 532	578
C	CyQ	PE-Cy5.18	488, 532	667
A	APC		595, 633, 635, 647	660
PC	PerCP		488, 532	678
PCC	PerCP-Cy5.5		488, 532	695



IQ Products BV  
Rozenburglaan 13a  
9727 DL Groningen, The Netherlands

 +31 (0)50 57 57 000  
 +31 (0)50 57 57 002  
 Technical [marketing@iqproducts.nl](mailto:marketing@iqproducts.nl)  
 Orders [orders@iqproducts.nl](mailto:orders@iqproducts.nl)  
 [www.iqproducts.nl](http://www.iqproducts.nl)